





SIGMOIDA ANALYSIS SOFTWARE

- Automated result interpretation
- Reporting in 2 seconds
- The **offline** software ensures data safety
- Automated report transfer to the Laboratory Information Systems.
- Human error elimination
- Ready-to-use for multiple kits

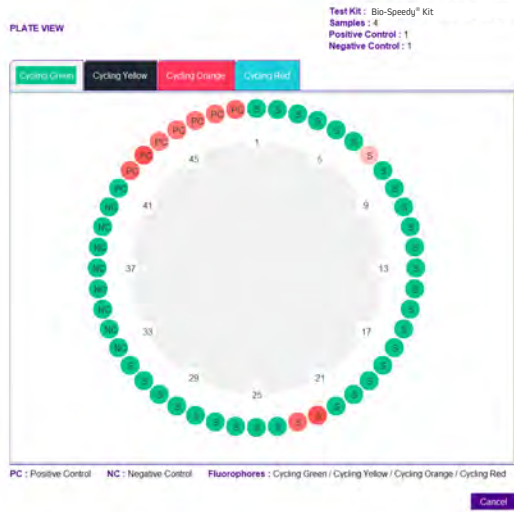

Mic qPCR Cyclar Plate Setup Interface

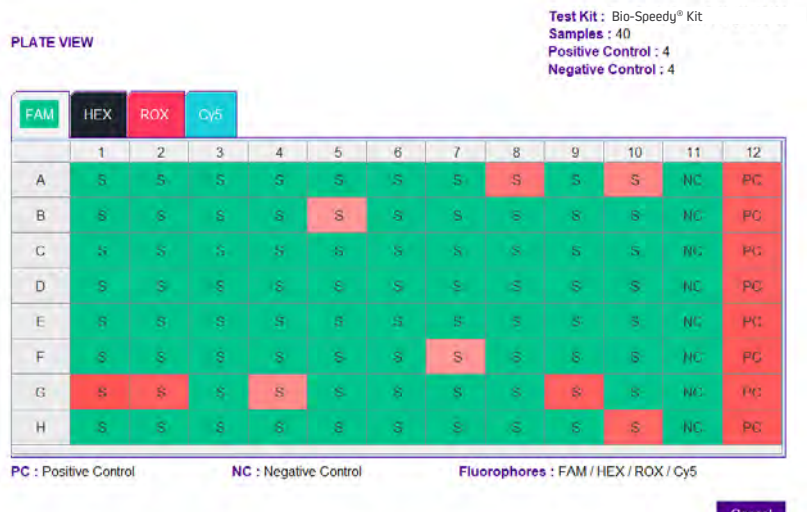

Bio-Rad Plate Setup Interface

Report

Test Kit : Bio-Speedy® Kit

File : CVD FLU DATA 1.pcrd

Date : 03 Feb 2023 09:10:22

User : Admin

Version : V 2.1.3

Show in plate view

All (171)Positive (37)Negative (101)Issues (33)Controls (39)

☒ Select All

	Well	Sample	Target	Cq	Result	Warnings
☒	A1	CVD HASTA 1	SARS-CoV-2	22.32	Positive	
☒	A1	CVD HASTA 1	Influenza B	N/A	Negative	
☒	A1	CVD HASTA 1	Influenza A	N/A	Negative	
☒	B1	CVD HASTA 1	SARS-CoV-2	24.04	Positive	
☒	B1	CVD HASTA 1	Influenza B	N/A	Negative	
☒	B1	CVD HASTA 1	Influenza A	N/A	Negative	
☒	D1	INF A HASTA 1	SARS-CoV-2	N/A	Negative	
☒	D1	INF A HASTA 1	Influenza B	N/A	Negative	
☒	D1	INF A HASTA 1	Influenza A	N/A	Negative	
☒	E1	INF B HASTA 1	SARS-CoV-2	N/A	Negative	
☒	E1	INF B HASTA 1	Influenza B	N/A	Negative	
☒	E1	INF B HASTA 1	Influenza A	N/A	Negative	
☒	A2	CVD HASTA 2	SARS-CoV-2	25.2	Positive	
☒	A2	CVD HASTA 2	Influenza B	N/A	Negative	
☒	A2	CVD HASTA 2	Influenza A	N/A	Negative	
☒	B2	CVD HASTA 2	SARS-CoV-2	24.81	Positive	
☒	B2	CVD HASTA 2	Influenza B	N/A	Negative	
☒	B2	CVD HASTA 2	Influenza A	N/A	Negative	

Result Reporting Table